

The TOMOX instrument: an x-rays tomographer for planetary applications

Lucia Marinangeli

Dep. of Psychological, Health & Territorial Science (DiSPuTer), Univ. G. d'Annunzio, Chieti, Italy

e-mail: lucia.marinangeli@unich.it

A.C. Tangari, L. Pompilio, A. Baliva

Dep. of Psychological, Health & Territorial Science (DiSPuTer), Univ. G. d'Annunzio, Chieti, Italy

M. Alvaro, M.C. Domeneghetti

Univ. Pavia, Italy

F. Frau, M.T. Melis

Univ. Cagliari, Italy

G. Bonanno, M.C. Rapisarda

INAF-Catania observatory, Italy

S. Pirrotta


Italian Space Agency, Rome, Italy

Abstract: The TOMOX instrument has been founded under the Italian Space Agency ASI DC-EOS-2014-309 call. TOMOX is thought to acquire both X-ray fluorescence and diffraction measurements from a sample in order to: a) achieve its chemical and mineralogical composition; b) reconstruct a 3D tomography of the sample exposed surface; c) give hints regarding the sample age. Nevertheless, this technique has applicability in several disciplines other than planetary geology, especially archaeology.

The word 'tomography' is nowadays used for many 3D imaging methods, not just for those based on radiographic projections, but also for a wider range of techniques that yield 3D images. Fluorescence tomography is based on the signal produced on an energy-sensitive detector, generally placed in the horizontal plane at some angle with respect to the incident beam caused by photons coming from fluorescence emission. So far, a number of setups have been designed in order to acquire X-rays fluorescence tomograms of several different sample types.


The proposed instrument is based on the MARS-XRD heritage. MARS-XRD is a project developed for the ESA ExoMars mission. The MARS-XRD instrument concept is based on a reflection geometry of acquisition for simultaneous measurements of diffracted and fluorescent X-rays. The breadboard includes a radioactive X-rays source (^{55}Fe) and n. 4 E2V CCDs 42-10, arranged along a curved ceramic structure of 12cm radius. Differently, TOMOX will use two different X-rays sources and two different detectors. Therefore, the novel arrangement has to be investigated.

The general idea of TOMOX is to distribute both sources and detectors along a moving hemispherical support around the target sample. As a result, both sources move integrally with the detectors while the sample is observed from a fixed position, thus preserving the geometry of observation. In that way, the whole sample surface is imaged and XRD and XRF measurements are acquired continuously along all the scans.

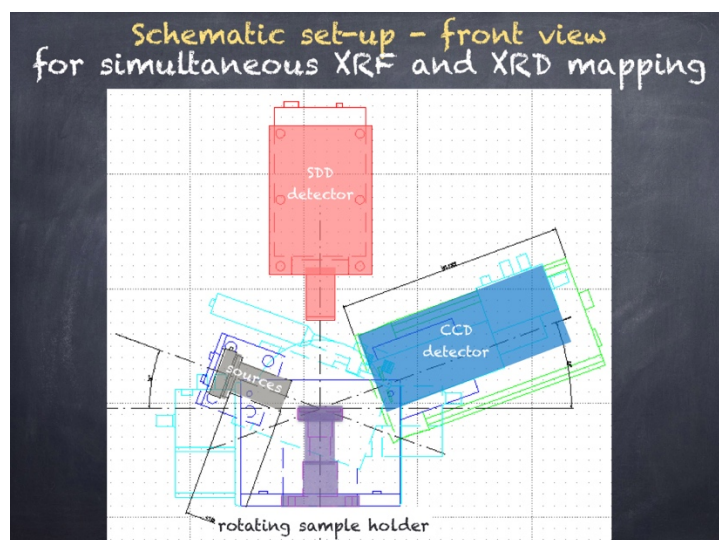

We plan to irradiate the target sample with X-rays emitted from ^{55}Fe and ^{109}Cd radioactive sources. ^{55}Fe and ^{109}Cd radioisotopes are commonly used as X-ray sources for analysis of metals in soils and rocks. The excitation energies of ^{55}Fe and ^{109}Cd are 5.9 keV, and 22.1 and 87.9 keV, respectively. Therefore, the elemental analysis ranges are Al to Mn with K lines excited with ^{55}Fe ; Ca to Rh, with K lines excited with ^{109}Cd . ^{55}Fe will be primarily dedicated to XRD measurements, as it has been already tested for the MARS-XRD development. ^{109}Cd will be used to reinforce the efficiency of ^{55}Fe source in the production of fluorescent X-rays generated in the sample as a consequence of irradiation and to extend the analytical range of elements.

Analogously, two separate detectors will be used in order to increase the total amount of events collected and allow the spatial distribution of events to be recorded as well. The detectors we plan to use are SDD (Silicon Drift Detector) and stand-alone CCD (Coupled Charge Detector). SDD has high count rate and stability and has been successfully used for XRF applications. CCD is able to record the spatial position of each event of X-ray emission, together with its energy. Therefore, we plan to dedicate this detector to XRD measurements, where the spatial position of the event is directly correlated to the type of crystal through the Bragg's law.

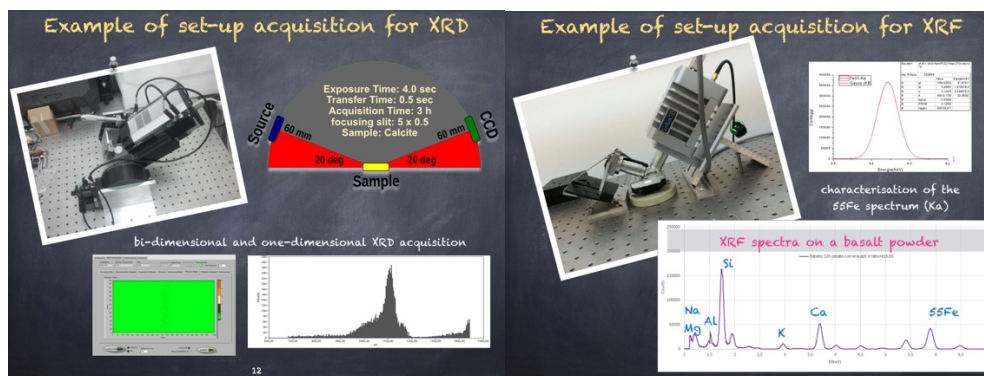

We are currently performing experimental tests for the sensors characterisation and signal calibration using different types of rock samples. Afterward, we will focus on the merging of XRD and XRF measurements to obtain the 3D tomographic modelling.

An appropriate mechanical design will be also developed to mount sources and sensors with movements to acquire in tomography mode.

References:

- [1] Marinangeli et al.. The mineralogy and chemistry analyser (MARS-XRD) for the ExoMars 2018 mission. EPSC-DPS Joint Meeting 2011, held 2-7 October 2011 in Nantes, France., 2011
- [2] Marinangeli, L.; Pompilio, L.; Baliva, A.; Bonanno, G.; Domeneghetti, M.C.; Fioretti, A.M.; Nestola, F.; Piluso, E.; Pondrelli, M.; Tateo, F. & the XMAP team. Development of an ultraminiaturized XRD/XRF instrument for the in situ mineralogical and chemical analysis of planetary soils and rocks and implication for Archeometry, Congresso Congiunto SGI-SIMP, Milano 10-12 Settembre 2014.
- [3] Marinangeli, Lucia, et al. "Development of an ultra-miniaturised XRD/XRF instrument for the in situ mineralogical and chemical analysis of planetary soils and rocks: implication for archaeometry." Rendiconti Lincei 26.4 (2015): 529-537, 2015